



PURE AND APPLIED CHEMISTRY INTERNATIONAL CONFERENCE 2020

**CHEMISTRY FOR CATALYZING
SUSTAINABILITY AND PROSPERITY**

FEBRUARY 13 - 14, 2020

**IMPACT FORUM, MUANG THONG THANI
NONTABURI, THAILAND**



Proceedings

The Pure and Applied Chemistry International
Conference 2020 [PACCON2020]
“Chemistry for Catalyzing Sustainability and Prosperity”
February 13-14, 2020

at

IMPACT Forum, Muangthong Thani, Nonthaburi, Thailand

Organized by

The Chemical Society of Thailand under the Patronage of Professor Dr. Her
Royal Highness Princess Chulabhorn Krom Phra Srisavangavadhana

In association with

Department of Chemistry, Faculty of Science and Technology
Thammasat University

Proceedings of the Pure and Applied Chemistry
International Conference 2020 [PACCON2020]

Editor-in-Chief Peerasak Paoprasert

Prepared by Department of Chemistry, Faculty of Science and Technology,
Thammasat University

1st Edition May 2020 [available in PDF file only]

Editorial Information

Editor-in-Chief Peerasak Paoprasert

Editorial Board see PACCON2020 Scientific Committee

Editorial Staff Chanatip Samart
Napaporn Youngvises
Sa-ad Riyajan
Yuthana Tantirungrotechai
Boonchoy Soontornworajit
Panumart Thongyoo
Natee Sirisit
Jatuporn Teerakul

SCIENTIFIC SESSIONS:

AC Analytical Chemistry

[Table of content](#)
[Proceedings](#)

CB Chemical Biology and Natural Products



Analytical Chemistry (AC)

Content	Page
Development of paper-based colorimetric sensor for determination of Human Papillomavirus DNA	AC1-AC7
Sarida Naorungroj, Prinjaporn Teengam, Tirayut Vilaivan, Orawon Chailapakul	
Development of paper-based biosensor using pyrrolidinyl PNA for screening of Hepatitis C virus DNA	AC8-AC14
Narathorn Nisab, Prinjaporn Teengam, Tirayut Vilaivan, Orawon Chailapakul	
Multiplexed simultaneous metal measurements using janus electrochemical paper-based analytical devices in particulate matter	AC15-AC21
Jaruwan Mettakoonpitak, Sookpichaya Charrunchon, John Volckens, Charles S. Henry	
Development and validation of HPLC method for simultaneous quantitative determination of amlodipine besylate and valsartan	AC22-AC28
Narisa Rukdee, Sutthikan Sonchai	
Chemometrics-assisted UV spectrophotometric methods for simultaneous determination of amlodipine besylate and valsartan in pharmaceutical tablets	AC29-AC34
Nidthida Archeepsudjarit, Supavadee Timum	
Quantitative determination of N-nitrosodimethylamine by HPLC method	AC35-AC40
Chutima Phechkrajang, Chaweewan Suwanvecho, Suttikan Sonchai, Narisa Rukdee, Nidthida Archeepsudjarit, Supavadee Timum	
Enantiomeric separation of chiral amines by GC using acetylated beta-cyclodextrin as stationary phase	AC41-AC46
Suchada Muangsri, Aroonsiri Shitangkoon	
Method development for determination of brominated flame retardants in high-impact polystyrene using X-ray fluorescence spectrometry	AC47-AC51
Polwat Singhasemanont, Apichat Imyim	
Development of Pb²⁺ electrochemical sensor using poly (diallyldimethylammonium chloride) @graphene dispersed chitosan modified glassy carbon electrode	AC52-AC56
Weenus Chaiprasert, Anchana Preechaworapun, Tanin Tangkuaram	
Fabrication of bimetallic of platinum-gold at poly-(diallyldimethylammonium chloride) modified graphene for application on the choline biosensors	AC57-AC61
Nuenghathai Chaiya, Anchana Preechaworapun, Tanin Tangkuaram	
The qualitative analysis of gamma-oryzanol in rice bran oil by using Raman spectroscopy	AC62-AC67
Pawida Sunghad, Chutima Phechkrajang, Pattamapan Lomarat, Somnuk Bunsupa, Bhanubong Bongcheewin, Natthinee Anantachoke	

Analytical Chemistry (AC)

Optimization of acrylamide analysis in flour sample by high performance liquid chromatography equipped with UV detector	AC68-AC73
Konkanok Jamsawang, Tinnakorn Tiensing	
Development and validation of a liquid chromatography tandem mass spectrometry method for the determination of 11-nor-9-carboxy-delta(9)-tetrahydrocannabinol in urine	AC74-AC79
Sirijit Jongjityotin, Anongphan Junkuy, Pongruk Sribanditmongkol, Chaturong Kanchai	
Cost-effective transparency sheet-based analytical device for colorimetric detection of folic acid	AC80-AC84
Ananyaporn Anekrattanasap, Weena Siangproh	
Detection of persulfate by gold nanorods multicolor sensor	AC85-AC89
Petrada Chunnuan, Charoenkwan Kraiya, Luxsana Dubas, Wanlapa Aeungmaitrepirom	
Transparency sheet-based colorimetric device using modified silver nanoparticles for the simple, sensitive and selective detection of calcium (II) ion	AC90-AC95
Paweenar Duenchay, Wijitar Dungchai	
Sensitive amperometric xylose detection with pyranose-2-oxidase-modified platinum electrodes	AC96-AC101
Nuttanun Kutrakul, Pangrum Punthong, Thanyaporn Wongnate, Pimchai Chaiyen, Albert Schulte	
Synthesis of gold nanoparticles-embedded bacterial cellulose nanopaper for colorimetric detection of hydrogen peroxide	AC102-AC107
Pongpichet Srikritsada Wong, Munlika Prommajun, Aurachat Lert-itthiporn, Saranya Phunpruch, Nathawut Choengchan	
Determination of arsenic (III) in soil using membraneless vaporization unit coupled with flow based system	AC108-AC113
Supattra Yooram, Piyada Jittangprasert, Kriangsak Songsrirote, Nuanlaor Ratanawimarnwong	
Spectrophotometric determination of gluconic acid in skincare products	AC114-AC119
Sophika Srihirun, Nuanlaor Ratanawimarnwong	
Chitosan cryogel incorporated with Prussian blue modified screen-printed carbon electrode for amperometric histamine biosensor	AC120-AC124
Natha Nontipichet, Suntisak Khumngern, Panote Thavarungkul, Proespichaya Kanatharana, Apon Numnuam	
Simple analytical method based on thin-layer chromatography imaging with mobile phone for determination of aflatoxin	AC125-AC128
Pantakarn Singchai, Jaroon Jakmune, Somkid Pencharee, Chanida Puangpila	

Analytical Chemistry (AC)

Determination of cordycepin and adenosine in Cordyceps militaris by high-performance liquid chromatography	AC129-AC133
Nutchanard Tumtamai, Sirikwan Ponprateep, Siritron Samosorn, Piyada Jittangprasert	
Pulsed amperometric detection of payload release from polymer nanoparticles	AC134-AC139
Piyanuch Vibulcharoenkitja, Yupaporn Niyo, Naruphorn Dararatana, Farzad Seidi, Albert Schulte, Daniel Crespy	
Flow injection system for detection of albumin based on gold nanoparticles-catalyzed luminol chemiluminescence	AC140-AC145
Bhoonnarasa Kasetsoontorn, Nathawut Choengchan	
Evaluation of stepwise constant current coulometric titration with potentiometric endpoint detection for sulfite determination	AC146-AC10
Chonnatee Tinala, Tinakorn Kanyanee	
Development of test kit for naked eye detection of sulfate in soil for brick manufacture	AC151-AC156
Arjnarong Mathaweensurn, Suprani Songsaeng, Rosemary Pongputh Kanyapak Thangjitsirisin, Sirirat Surasen, Nuanlaor Ratanawimarnwong, Nathawut Choengchan	
Planar contactless conductivity detector with paper as liquid reservoir: cell geometry and applications	AC157-AC162
Nutnaree Fukana, Thitaporn Sonsa-ard, Nattapong Chantipmanee, Prapin Wilairat, Peter C. Hauser, Duangjai Nacapricha	
The magnetic solid-phase extraction for determination of lead (II) ion in contaminated wastewaters using flow injection amperometry	AC163-AC168
Sakkarin Phumma, Suthipong Puangthong, Manoch Thanomwat, Sakchai Satienerakul	
Direct image analysis of gunshot residue on white fabric target: comparison with an extraction method with colorimetric paper-based method for the estimation of shooting distance	AC169-AC173
Thinnapong Wongpakdee, Supatana Buring, Phoonthawee Saetear, Nuanlaor Ratanawimarnwong, Kanchana Uraisin, Prapin Wilairat, Warawut Tiyapongpattana, Duangjai Nacapricha	
Boron and nitrogen doped graphene for electrochemical detection of glutathione	AC174-AC179
Tanyapone Purttisarikorn, Wijitra Dungchai	
Analysis of arsenic speciation in drinking water by capillary electrophoresis	AC180-AC184
Khajadpai Thipyapong, Somsak Sirichai	

Analytical Chemistry (AC)

Colorimetric detection of Salmonella typhimurium in food using gold nanoparticles on paper-based device	AC185-AC190
Wanida Wonsawat, Sripeth Thongkaow, Sunisa Limvongjaroen, Nalin Ratnarathorn, Wijitar Dungchai	
Environmental friendly electrochemical sensor based on of Bi/poly(L-cys)/GCE for zinc detection	AC191-AC195
Anisah Dueraning, Sayan Tansuan, Nattanicha Jaturaphet, Maneetip Phonpakdee, Nattakon Cheeprawatchai, Darin Boonsri, Porntip Supatchaiyawong, Supaporn Dawan	
Flow injection titration at non-steady state for determination of acetic acid	AC196-AC200
Wanida Loetsaksrisakul, Natcha Kaewwonglom, Jantima Upan, Jaroon Jakmune	
Metabolomics approach revealed the different metabolic profiles of Aspergillus species by HPLC-MS	AC201-AC206
Worawut Chaiyasaeng, Jamrearn Buaruang, Boon-ek, Yingyong narongkul	
Characterization of methacrylate-based monolithic materials synthesized in pipette tip for micro-solid phase extraction	AC207-AC212
Kesara Ar-sanork, Apiwat Muekhunthod, Ati Chetsurakul, Chanpen Karuwan, Nakin Surapanich, Patcharin Chaisuwan	
Electrospun polyacrylonitrile/graphene oxide nanofibers as sorbent for solid phase extraction	AC213-AC219
Chotitas Sribun, Puttaruksa Varanusupakul	
A non-destructive technique for determination of thorium concentration in geological samples using gamma spectrometry	AC220-AC224
Paphon Phaukkachane, Saowaluck Thong-in, Kalaya Changkrueng, Harinate Mungpayaban	

Anisah Dueraning^{1*}, Sayan Tansuan², Nattanicha Jaturaphet¹, Maneetip Phonpakdee¹,
Nattakon Cheeprawatchai¹, Darin Boonsri¹, Porntip supatchaiyawong¹, Supaporn Dawan¹

¹*Department of Chemistry, Faculty of Education, Phuket Rajabhat University, Phuket 83000,
Thailand*

²*Department of Chemistry, Faculty of Science and Technology, Phuket Rajabhat University,
Phuket 83000, Thailand*

**E-mail: Anisah.d@pkru.ac.th*

Electrochemical sensors based on bismuth modified poly (L- cysteine) / glassy carbon electrode (Bi-poly(L-cys)/GCE) as an environmentally-friendly electrode to detect zinc by anodic stripping voltammetry. Bi film was prepared by an in situ plating of bismuth onto the poly(L-cys)/GCE. The operational parameters such as L- cysteine concentration, bismuth concentration, preconcentration potential, and preconcentration time were optimized. Under the optimum conditions, the sensitivity of the Bi-poly(L-cys)/GCE higher than the bare GCE, Bi/GCE, and poly(L-cys)/GCE was 8.5, 6.3, and 3.6 times respectively. The linear range was 0.005-0.100 mg L⁻¹ (r = 0.999) with a detection limit of 0.002 mg L⁻¹ and a quantitation limit of 0.008 mg L⁻¹. This method could possibly be applied to determine zinc in real samples such as food, soil, and wastewater.

Keywords: Anodic stripping voltammetry; Zinc; L- cysteine; Bi- poly(L- cys) / GCE; Environmentally-friendly

Environmental friendly electrochemical sensor based on of Bi/poly(L-cys)/GCE for zinc detection

Anisah Dueraning^{1*}, Sayan Tansuan², Nattanicha Jaturaphet¹, Maneetip Phonpakdee¹, Nattakon Cheeprawatchai¹, Darin Boonsri¹, Porntip Supatchaiyawong¹, Supaporn Dawan¹

¹Department of Chemistry, Faculty of Education, Phuket Rajabhat University, Phuket 83000, Thailand

²Department of Chemistry, Faculty of Science and Technology, Phuket Rajabhat University, Phuket 83000, Thailand

*E-mail: Anisah.d@pkru.ac.th

An environmentally-friendly electrochemical sensors based on bismuth modified poly(L-cysteine) / glassy carbon electrode (Bi/poly(L-cys)/GCE) has been developed to detect zinc ion by anodic stripping voltammetry. The Bi film was prepared by an in situ plating of bismuth onto the poly(L-cys)/GCE. The operation parameters such as L-cysteine concentration, bismuth concentration, preconcentration potential, and preconcentration time were optimized. Under the optimum conditions, the sensitivity of the modified electrodes (Bi/poly(L-cys)/GCE, Bi/GCE, and poly(L-cys)/GCE) compared with the bare GCE was 8.5, 6.3 and 3.6 times respectively. The linear range was 0.005-0.100 mg L⁻¹ (r = 0.999) with a detection limit of 2.0 µg L⁻¹ and a quantitation limit of 8.0 µg L⁻¹. This method showed a potential be applied for zinc ion determination in real samples such as food, soil, and wastewater

1. Introduction

Zinc (Zn) is an essential nutrient for the growth, it is an important trace element needed by plants in small amounts, but yet crucial to plant development. In plants, Zn is a key constituent of many enzymes and proteins. In the case of soil that has too much phosphorous (P) or phosphate (PO₄³⁻), will lead to zinc deficiency in soils due to the formation of insoluble zinc phosphate (Zn₃(PO₄)₂) resulting in plants absorb less zinc.¹ However, zinc deficiency frequently found in almost all plants and it is a common problem in agricultural land around the world.

The normally methods were used to determine zinc as atomic absorption spectrophotometry (AAS) and inductively coupled mass spectrometry (ICP-MS). There provided high accuracy, precision and sensitivity, however they require expensive instrumentation, have high operating costs with long analysis time.² The anodic stripping voltammetry (ASV) technique was interesting, because it can provide a high sensitivity, low

detection limit, reduced consumption of chemical and sample, and short analysis time.^{3,4} For determination of metal ions by ASV in the past mainly used mercury electrodes.⁵ However, mercury is highly toxic and can be harmful to researchers, users, and the environment, therefore analytical methods that are used glassy carbon electrode (GCE) more environmentally friendly and safe for the operator are being developed based on the concept of green chemistry.⁶ Various materials with electrical properties are improve the GCE such as graphene.⁷ Graphite.⁸ and multiwalled carbon nanotube (MWCNTs).⁹ Then polymer film modified electrodes using the electropolymerization technique have been considered to be an attractive due to its good stability, homogeneity and good adhesion to the electrode surface, insolubility, increased surface area, and more active sites.^{10,11} This work to used GCE as an environmental friendly electrode, it was fabricated by electropolymerization. Bismuth film (BiF) was prepared by an in situ plating of bismuth onto the poly(L-cys)/GCE for determination

of zinc by ASV. The effect of several operational parameters were studied consisted of L-cysteine concentration, bismuth concentration, preconcentration potential, and preconcentration time, linear range, limit of detection (LOD) and limit of quantitation (LOQ), repeatability.

2. Materials and Methods

2.1 Materials

L-cysteine, bismuth(III) nitrate pentahydrate, zinc acetate dihydrate, and sodium acetate trihydrate were from Ajax finechem (Australia). Acetic acid, hydrochloric acid and nitric acid were from Biolabo (France). All other chemical were of analytical grade. Buffers were prepared with deionized water. Before use, buffer was filtered through a Millipore filter.

2.2 Apparatus

The electrochemical techniques were carried out in a conventional three-electrode cell controlled by 910 PSTAT mini potentiostat (Metrohm Autolab B. V., The Netherlands). Glassy carbon electrode (GCE; diameter 3.0 mm) was used as the working electrode. A silver/silver-chloride electrode (Ag/AgCl) and a platinum wire were used as a Reference electrode and counter electrode, respectively. The pH measurements were performed at a S220 pH meter (Mettler-toledo, Switzerland).

2.3 Fabrication of poly(L-cys)/GCE

The working electrode was first polished with 1.5, 0.5, and 0.05 μm alumina powder and washed with deionized water. The cleaned electrode was immersed in 0.05 mM L-cys in 0.1 M HCl for 10 cycles of potential sweep between -1.2 and +1.8 V at a scan rate 0.1 V s^{-1} . The poly(L-cys)/GCE

was then gently washed with water and dried at room temperature.

2.4 ASV measurement

The three-electrode system consisted of a working electrode as modified with poly(L-cys), Reference electrode and counter electrode, were immersed in 0.10 M acetate buffer solution pH 4.5. Amount of Zn(II) and 1.0 mM Bi(III) were simultaneously deposited on the surface of the poly(L-cys)/GCE at -1.40 V for 120 s under stirring. Then the accumulation period, the stirring was stopped and after a 5 equilibrium time, the voltammogram was recorded using a square-wave potential scan between -1.40 and -0.80 V.

3. Results & Discussion

3.1 Optimization of electrode modification

The effect of L-cysteine concentration was studied between 0.010 and 0.075 mM in 0.1 M HCl (Figure 1. (a)) potential scan from -1.2 to +1.8 V, 10 cycles at scan rate 0.1 Vs^{-1} by cyclic voltammetry (CV). When tested with Zn(II) the sensitivity increase with concentration from 0.010 to 0.050 mM, and then decreased. This may be because poly(L-cys) film at GCE surface is too thick, it will have blocked the electron transfer.¹² The concentration of L-cys at 0.050 mM was chosen to study the next parameters.

The numbers of cycles for electropolymerization of poly(L-cys) at the GCE surface were investigated, between 5 and 25 cycles (Figure 1b). After that tested with Zn(II) the sensitivity increase with number of cycles from 5 to 15, and then decreased. This may be because poly(L-cys) film at GCE surface is too thick, this caused inhibition of electron transfer on the surface.¹³ Therefore, electropolymerization of poly(L-cys) at 15 cycles was used for further studied

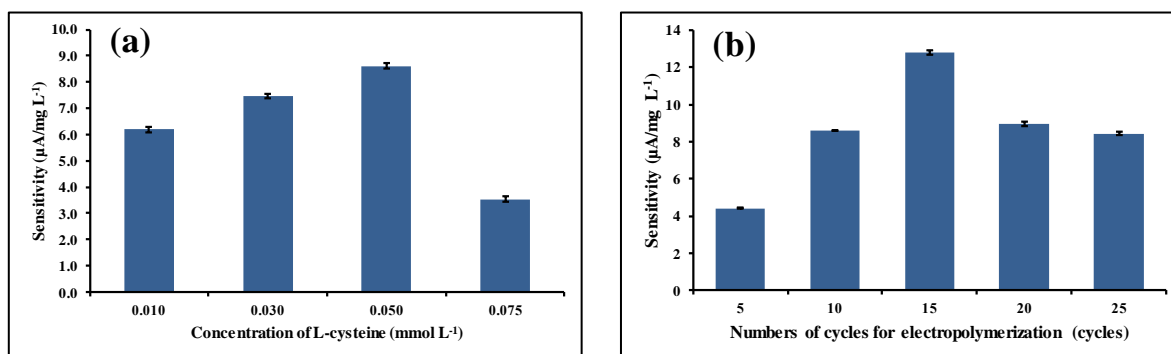


Figure 1. The effect of L-cysteine concentration (a) on the sensitivity of the fabrication electrode and Effect of the numbers of cycles for the electropolymerization (b) of the poly(L-cys) at the GCE surface. The sensitivity is slope of the calibration curve at the concentration of Zn(II) between 0.05 and 0.50 mg L⁻¹. (ASV operation conditions: 60 s preconcentration time, -1.40 V preconcentration potential with stirring, square-wave potential scan between -1.40 and -0.50 V).

3.2 Optimization of the operational conditions for zinc detection

The concentrations of bismuth were studied, between 0.10 and 2.0 mM at the potential -1.4 V for 60 s in acetate buffer pH 4.5. When the concentration increase the sensitivity increased up to 1.0 mM, the increasing of Bi(III) concentration increased the Bi film on the poly(L-cys)/GCE, and resulted in the increasing of Bi-Zn alloying on the electrode surface, thus, increased the anodic peak current. However, the sensitivity decreased when the Bi(III) concentration was higher than 1.0 mM, it probably because Bi(III) film is too thick, it will hold back the Zn and affect the anodic peak current of Zn during the stripping step.¹⁴

The effect of preconcentration potential was studied, from -1.20 to -1.60 V, 60 s in acetate buffer pH 5.0 (Figure 2a). The

sensitivity increased as the preconcentration potential increased, between -1.20 and -1.40 V, and then the sensitivity decrease when preconcentration potentials higher than -1.40 V, it may be because had hydrogen evolution on the electrode surface and inhibited Zn(II) accumulation step to affect the sensitivity reduce¹⁵. Therefore, at -1.20 V was chosen for preconcentration potential.

The effect of preconcentration time was studied in the range of 30 to 240 s, potential -1.40 V, acetate buffer pH 5.0 (Figure 2b). The sensitivity was increased from 30 to 120 s, and then decreased at the preconcentration time higher than 120 s, this may be because poly(L-cys) film at GCE surface is too thick, this caused inhibition of electron transfer on the surface.¹³ Therefore, the preconcentration time at 120 s was chosen.

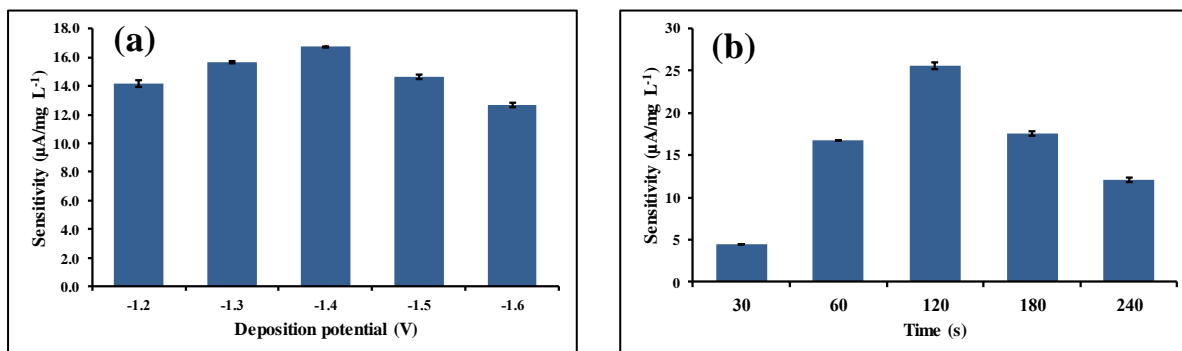


Figure 2. The effect of preconcentration potential (a) and The effect of preconcentration time (b) on the sensitivity of Zn(II) on the Bi/poly(L-cys). The sensitivity is slope of the calibration curve at the concentration of Zn(II) between 0.05 and 0.50 mg L⁻¹. (ASV operation conditions: 60 s preconcentration time, -1.40 V preconcentration potential with stirring, square-wave potential scan between -1.40 and -0.50 V).

3.3 Calibration curve, detection limit and quantitation limit

Under the optimum conditions, the linear range was 0.005 to 0.100 mg L⁻¹ ($r = 0.999$) (Figure 3). The detection limit (LOD) and the quantitation limit (LOQ) were calculated as 2.0 µg L⁻¹ and 8.0 µg L⁻¹, respectively, by using the equation $LOD = 3S_a/b$ and $LOQ = 10S_a/b$, S_a is the standard deviation of the intercept and b is the slope of the calibration curve¹⁶. Then the sensitivity of the modified electrodes (Bi/poly(L-cys)/GCE, Bi/GCE, and poly(L-cys)/GCE) compared with the bare GCE was 8.5, 6.3, and 3.6 times respectively.

4. Conclusions

This work, glassy carbon electrode has been modified with poly(L-cys) and was used to detected zinc by anodic stripping voltammetry through an *in situ* plating onto the poly(L-cys)/GCE. The detection provided high sensitivity and low detection limit. The Bi/poly(L-cys)/GCE is environmentally friendly and showed a potential be applied for zinc ion determination in real samples such as food, soil, and wastewater.

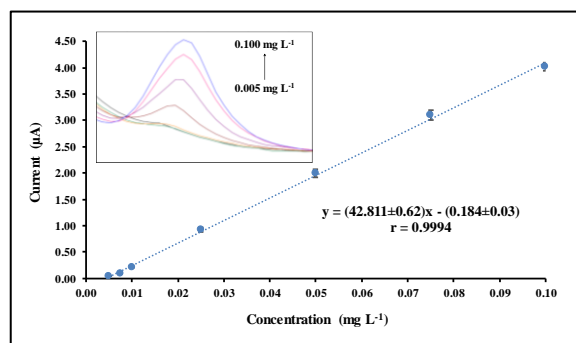


Figure 3. The calibration curve between the anodic peak current and the concentration of Zn(II) in the range from 0.005 to 0.100 mg L⁻¹. The inset shows the anodic stripping voltammograms of Zn(II).

Acknowledgements

This research was supported by Chemistry department, faculty of Education, and faculty Science and Technology, Phuket Rajabhat University. Special thanks to Asst. Prof. Dr. Warakorn Limbut for giving a great opportunity to work and excellent guidance.

References

- Ahmad, P. Water Stress and Crop Plants: A Sustainable Approach (Vol 1). 1st ed. Chichester, UK. John Wiley & Sons, Ltd. 2016.

- Xu, H.; Zeng, L.; Huang, D.; Xian, Y.; Jin, L. *Food Chem.* **2008**, *109*, 834-839.
- Wang, J. *Analytical Electrochemistry*. 2nd ed. Third Avenue, New York, NY. John Wiley & Sons, Inc. 2000.
- Willemse, C.M.; Thhomelang, K.; Jahed, N.; Baker, P.G.; Iwuoha, E.I. *Sensors*. **2011**, *11*, 3970-3987.
- Trindade, J. M. ; Martiniano, L. C. ; Gonçalves, V. R. A. ; Souza, A. G. ; Marques, A.L.B.; Baugis, G.L.; Fonseca, T.C.O.; Song, C.; Zhang, J.; Marques, E.P. *Fuel*. **2012**, *91*, 26-32.
- United States Environmental Protection Agency. Green Chemistry. <https://www.epa.gov/greenchemistry> (accessed January 3, 2019)
- Lee, S.; Bong, S.; Ha, J.; Kwak, M.; Park, S.-K.; Piao, Y. *Sensors Actuat. B.* **2015**, *215*, 62-69.
- Feier, B.; Floner, D.; Cristea, C.; Bodoki, E.; Sandulescu, R.; Geneste, F. *Talanta* **2012**, *98*, 152-156.
- Palisoc, S.; Vitto, R. I. M.; Natividad, M. *Sci Rep.* **2019**, *9*(18491), 1-13.
- Wei, Y.; Luo, L.; Ding, Y.; Liu, X.; Chu, Y. *Microchim Acta.* **2013**, *180*, 887-893.
- Rahman, Md. A.; Won, M.-S.; Shim, Y.-B. *Anal Chem.* **2003**, *75*, 1123-1129.
- Zhou, X.; Zheng, X.; Lv, R.; Kong, D.; Li, Q. *Electrochim. Acta.* **2013**, *107*, 164-169.
- Dueraning, A. ; Kanatharana, P. ; Thavarungkul, P. ; Limbut, W. *Electrochim Acta.* **2016**, *221*, 133-143.
- Wu, Y.; Li, N. B.; Luo, H, Q. *Sensors Actuat B.* **2008**, *133*, 677-681.
- Jothimuthu, P.; Wilson, R. A.; Herren, J.; Pei, X.; Kang, W.; Daniels, R.; Wong, H.; Beyette, F.; Heineman, W. R.; Papautsky, I. *Electroanal.* **2013**, *25*(2), 401-407.
- Swartz, M. E. ; Krull, I. S. *Analytical method development and validation*. 1st ed. Madison Avenue, New York, NY. Marcel Dekker, Inc. 1997.

